

CERTIFICATE OF ANALYSIS

Product: Monoclonal anti-S-Adenosylhomocysteine (SAH) antibody clone 839-12

Catalog Number: MA00308

Lot Number: Lot# MP421608, Lot#MP480213, Lot#MP451607, Lot#MP451219

Document Release Date: July 24, 2017


Test	Specification	Result
Appearance	Clear liquid	Clear solution
Concentration (by UV Spectrophotometer)	About 0.5-1mg/ml	About 0.5-1mg/ml
Storage buffer	10mM PBS pH 7.4 (150 mM NaCl), 0.02%NaN3	10mM PBS pH 7.4 (150 mM NaCl), 0.02%NaN3
Stability at 4°C	30 days	Same dilution in 48 days
Stability at -20°C	>1 year	>1 year
Stability at freeze and thaw	Avoid repeated freeze-and-thaw	No change in antigen-binding capability after freezer and thaw 10 times
Specificity	Cross reaction with SAM about <3%, other analogs < 1%	Cross reaction with SAM ~ 1.33%, other analogs < 1%
Sensitivity (by cELISA)	PBS: ~30nM Plasma: 62.5nM	PBS: ~30nM Plasma: 31.25 - 62.5nM
Affinity (by cELISA, see details below)	$K_a \geq 10^8$ L/mol	$K_a = 6.8 \times 10^9$ L/mol $= 1.47 \times 10^{-10}$ M
Titer (see curve below)	Adjust antibody at 1mg/ml	Suggested: 32,000 in cELISA

Specificity

Figure below showed a competitive ELISA using anti-S-Adenosylhomocysteine monoclonal antibody [839-12] (MA00308). The 0.2 µg/ml of SAH-BSA was coated into 96 wells. Serial dilution of SAH standard (SAHNa), S-Adosylmethionine (SAM: Sigma-Aldrich Cat# A2408), Homocysteine (H-Cys), L-Cysteine (L-Cys), Adenosine (Ade), Glutathione (GST), L-Cystathionine (L-CTT), Methythioadenosine (MTA), ADP (adenosine diphosphate), ATP (adenosine triphosphate) and properly diluted MA00305 were added. HRP conjugated Goat anti-Mouse IgG antibody was used to develop the color. OD450 value was


Products are warranted to operate or perform substantially in conformance with published product data sheet in effect at the time of sale, as set forth in the product documentation, specifications and/or accompanying package inserts ("Documentation"). Arthus Biosystems warrants at the time of release, this product conformed information contained in this certificate of analysis. The warranty provided herein is valid only when used by properly trained individuals. Unless otherwise stated in the Documentation, this warranty is limited to one year from date of shipment when the product is subjected to normal, proper and intended usage. The warranty extends only to the buyer of the product. Product is intended for research only and is not to be used for any other purpose, including unauthorized commercial uses, in vitro diagnostic uses, ex vivo or in vivo therapeutic uses, or any type of consumption by or application to humans or animals.

measured on each well. The relatively higher cross-reaction with SAM and MTA (<5%) should not be concerned as physiological levels of SAM and MTA are much lower than 1uM, at which level no cross reaction with the antibody is observed.

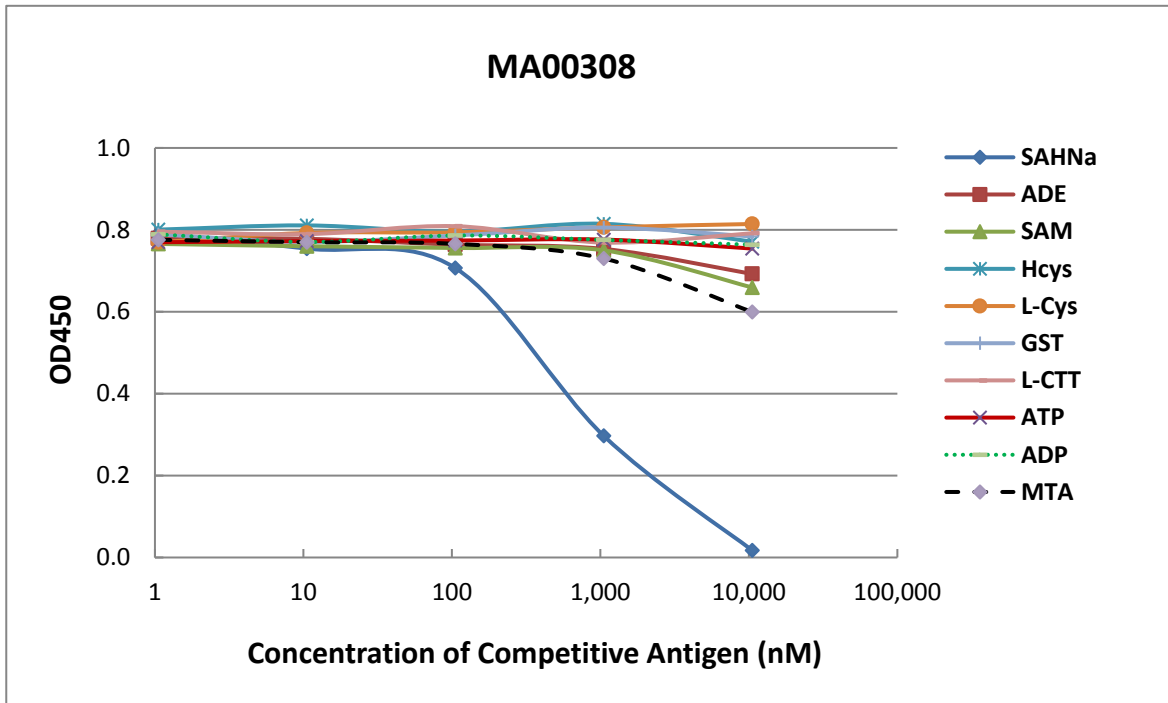

Titer

Products are warranted to operate or perform substantially in conformance with published product data sheet in effect at the time of sale, as set forth in the product documentation, specifications and/or accompanying package inserts ("Documentation"). Arthus Biosystems warrants at the time of release, this product conformed information contained in this certificate of analysis. The warranty provided herein is valid only when used by properly trained individuals. Unless otherwise stated in the Documentation, this warranty is limited to one year from date of shipment when the product is subjected to normal, proper and intended usage. The warranty extends only to the buyer of the product. Product is intended for research only and is not to be used for any other purpose, including unauthorized commercial uses, in vitro diagnostic uses, ex vivo or in vivo therapeutic uses, or any type of consumption by or application to humans or animals.

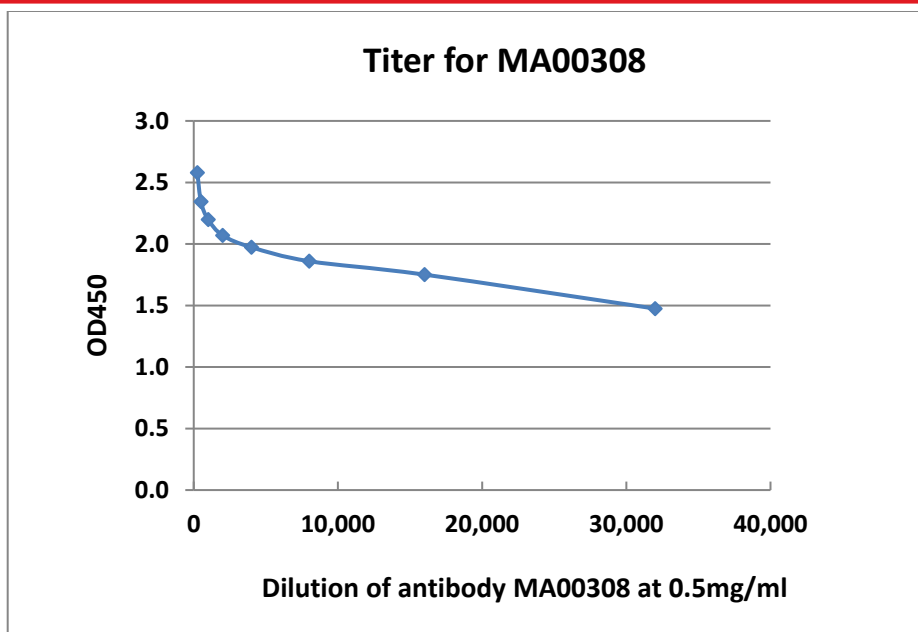

Affinity

Table 1 Anti-SAH Antibodies (839-12 at 1mg/ml) Binding to Different Amount of Antigen

Dilution	BSA-SAH 0.4ug/ml	BSA-SAH 0.2ug/ml
4000	4.02165	2.8649
8000	3.75655	2.7837
16000	3.489	2.5598
32000	2.92615	2.2305
64000	2.26735	1.8240
128000	1.5222	1.2943
256000	0.97805	0.8367
512000	0.59925	0.5158


From Table 1, when coating antigen was at 0.4µg/ml, half the maximum OD was seen at about 1:97452. The corresponding antibody concentration was $[Ab] = (1\text{mg/ml}/160,000\text{g/mol})/ 97452 = 6.41 \times 10^{-11} \text{ M}$, where 160,000 is the molecular weight of antibody. When coating antigen was at 0.2µg/ml, half the

Products are warranted to operate or perform substantially in conformance with published product data sheet in effect at the time of sale, as set forth in the product documentation, specifications and/or accompanying package inserts ("Documentation"). Arthus Biosystems warrants at the time of release, this product conformed information contained in this certificate of analysis. The warranty provided herein is valid only when used by properly trained individuals. Unless otherwise stated in the Documentation, this warranty is limited to one year from date of shipment when the product is subjected to normal, proper and intended usage. The warranty extends only to the buyer of the product. Product is intended for research only and is not to be used for any other purpose, including unauthorized commercial uses, in vitro diagnostic uses, ex vivo or in vivo therapeutic uses, or any type of consumption by or application to humans or animals.

maximum OD was observed at about 1: 113761. The corresponding antibody concentration was $[Ab]_t = (1\text{mg/ml}/160,000\text{g/mol})/ 113761 = 5.47 \times 10^{-11} \text{ M}$.

$n = 2$

$K_a = (n-1)/2 * (n[Ab] - [Ab]_t) = 6.8 \times 10^9 \text{ L/mol}$



Jimmy Li
Quality Control Team

Products are warranted to operate or perform substantially in conformance with published product data sheet in effect at the time of sale, as set forth in the product documentation, specifications and/or accompanying package inserts ("Documentation"). Arthus Biosystems warrants at the time of release, this product conformed information contained in this certificate of analysis. The warranty provided herein is valid only when used by properly trained individuals. Unless otherwise stated in the Documentation, this warranty is limited to one year from date of shipment when the product is subjected to normal, proper and intended usage. The warranty extends only to the buyer of the product. Product is intended for research only and is not to be used for any other purpose, including unauthorized commercial uses, in vitro diagnostic uses, ex vivo or in vivo therapeutic uses, or any type of consumption by or application to humans or animals.