

## CERTIFICATE OF ANALYSIS

**Product:** Monoclonal anti-S-Adenosylmethionine (SAM) antibody clone 118-18

**Catalog Number:** MA00203

**Lot Number:** Lot#MP422429, Lot#MP421815, Lot#MP421816, Lot#MP420825


**Document Release Date:** July 24, 2017

Test	Specification	Result
Appearance	Clear liquid	Clear solution
Concentration (by UV Spectrophotometer)	0.5 - 1 mg/ml	0.5 - 1mg/ml
Storage buffer	10mM PBS pH 7.4 (150 mM NaCl) , 10mg/ml BSA,0.02%NaN3, 50%Glycerol	10mM PBS pH 7.4 (150 mM NaCl) , 10mg/ml BSA,0.02%NaN3, 50%Glycerol
Stability at 37°C	Few hours	Same dilution in 14 days
Stability at 4°C	30 days	Same dilution in 48 days
Stability at -20°C	>1 year	>1 year
Stability at freeze and thaw	Avoid repeated freeze-and-thaw	No change in antigen-binding capability after freezer and thaw 14 times
Stability with dilution up to 5 folds	Diluted antibodies may be less stable	No difference during the period of thermal stability tests above
Specificity	Cross reaction with analogs <1%	Cross reaction with analogs <1%
Sensitivity (by cELISA)	PBS: 3nM; Plasma: 30-60nM	PBS: 3nM; Plasma: 30-60nM
Affinity (by cELISA, see details below)	$K_a \geq 10^9$ L/mol	$K_a = 7.68 \times 10^9$ L/mol $= 1.30 \times 10^{10}$ M

### Specificity


**(1)** Dosage-dependent competition was detected as a sample was added to a cELISA (Any SAM from a sample competes with the coated SAM heptan to bind HRP-conjugated antibody 118-18). The sample is the product of the following biochemical reaction: Methionine Adenosyltransferase (MAT) was added to methionine and adenosine triphosphate under an appropriate buffer at 37°C. It indicates that antibody 118-18 specifically binds physiologically produced SAM.

Products are warranted to operate or perform substantially in conformance with published product data sheet in effect at the time of sale, as set forth in the product documentation, specifications and/or accompanying package inserts ("Documentation"). Arthus Biosystems warrants at the time of release, this product conformed information contained in this certificate of analysis. The warranty provided herein is valid only when used by properly trained individuals. Unless otherwise stated in the Documentation, this warranty is limited to one year from date of shipment when the product is subjected to normal, proper and intended usage. The warranty extends only to the buyer of the product. Product is intended for research only and is not to be used for any other purpose, including unauthorized commercial uses, in vitro diagnostic uses, ex vivo or in vivo therapeutic uses, or any type of consumption by or application to humans or animals.

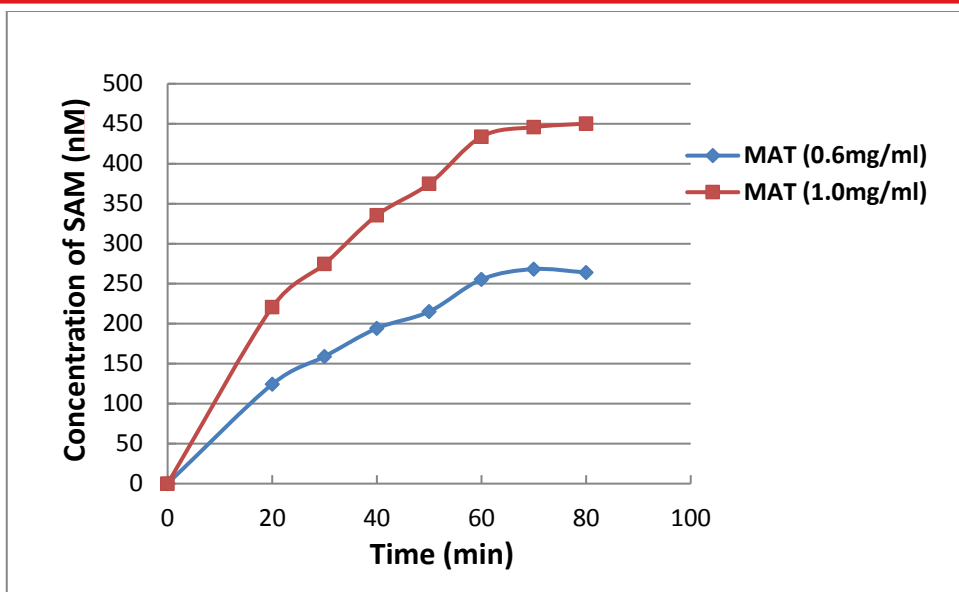

**(2) Cross reaction** Figure below showed a competitive ELISA using anti-S-Adenosymethionine monoclonal antibody [118-18] (MA00203). The 0.1  $\mu\text{g/ml}$  of SAM coating standard (Cat # ACT00203) was coated into 96 wells. Serial dilution of SAM standard (Cat # AST00203), S-Adenosylhomocysteine (SAH), Adenosine (Ade), L-Methionine (Met), Methythioadenosine (MTA), Adenosine diphosphate (ADP), Adenosine triphosphate (ATP) and 1:15000 of MA00203 were added. HRP conjugated Goat anti-Mouse IgG antibody was used to develop the color.

Products are warranted to operate or perform substantially in conformance with published product data sheet in effect at the time of sale, as set forth in the product documentation, specifications and/or accompanying package inserts ("Documentation"). Arthus Biosystems warrants at the time of release, this product conformed information contained in this certificate of analysis. The warranty provided herein is valid only when used by properly trained individuals. Unless otherwise stated in the Documentation, this warranty is limited to one year from date of shipment when the product is subjected to normal, proper and intended usage. The warranty extends only to the buyer of the product. Product is intended for research only and is not to be used for any other purpose, including unauthorized commercial uses, in vitro diagnostic uses, ex vivo or in vivo therapeutic uses, or any type of consumption by or application to humans or animals.

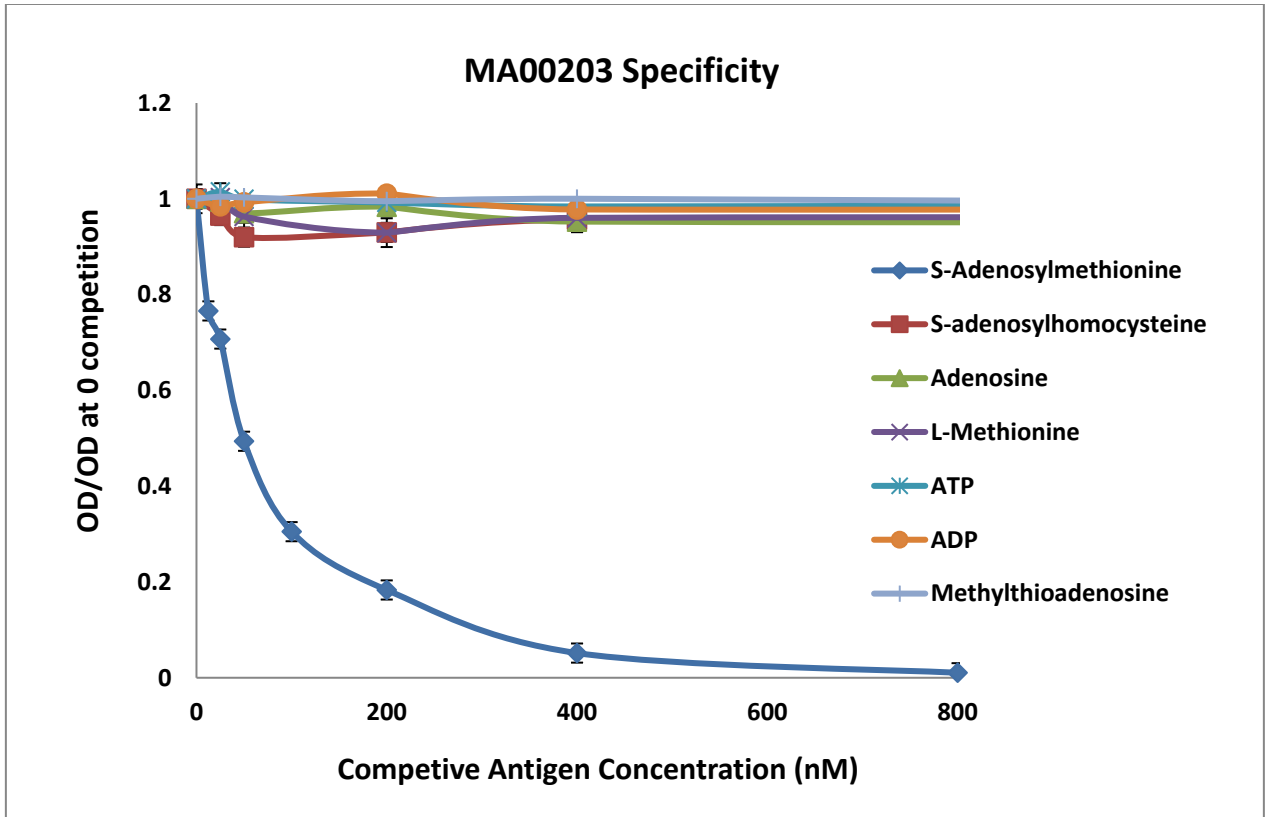

### Sensitivity

Similar to clone 118-6

### Affinity

Table 2 Anti-SAM Antibodies (118-18) Binding to Different Amount of Antigen

Dilution from 1mg/ml	Monoclonal anti-SAM 118-18 PLL-aza-SAM	
	0.05µg/ml	0.1µg/ml
1000	1.5046	2.5979
2000	1.4906	2.4437
4000	1.2725	2.3165
8000	1.1282	2.0831
16000	0.9172	1.7791

Products are warranted to operate or perform substantially in conformance with published product data sheet in effect at the time of sale, as set forth in the product documentation, specifications and/or accompanying package inserts ("Documentation"). Arthus Biosystems warrants at the time of release, this product conformed information contained in this certificate of analysis. The warranty provided herein is valid only when used by properly trained individuals. Unless otherwise stated in the Documentation, this warranty is limited to one year from date of shipment when the product is subjected to normal, proper and intended usage. The warranty extends only to the buyer of the product. Product is intended for research only and is not to be used for any other purpose, including unauthorized commercial uses, in vitro diagnostic uses, ex vivo or in vivo therapeutic uses, or any type of consumption by or application to humans or animals.

---


---

32000	0.7316	1.442
64000	0.5371	1.149
128000	0.4012	0.9416

From Table 2, when coating antigen was at 0.05µg/ml, half the maximum OD was seen at about 1:32000. The corresponding antibody concentration was  $[Ab]_t = (1\text{mg/ml}/160,000\text{g/mol})/32000 = 1.302 \times 10^{-10}\text{M}$ , where 160,000 is the molecular weight of antibody. When coating antigen was at 0.1µg/ml, half the maximum OD was observed at about 1:48000. The corresponding antibody concentration was  $[Ab] = (1\text{mg/ml}/160,000\text{g/mol})/48000 = 1.953 \times 10^{-10}\text{M}$ .

$$n = (0.1\mu\text{g/ml})/(0.05\mu\text{g/ml}) = 2$$

$$K_a = (n-1)/2 * (n[Ab] - [Ab]_t) = 7.68 \times 10^9 \text{L/mol} = 1.30 \times 10^{-10}\text{M}$$



Jimmy Li  
Quality Control Team

Products are warranted to operate or perform substantially in conformance with published product data sheet in effect at the time of sale, as set forth in the product documentation, specifications and/or accompanying package inserts ("Documentation"). Arthus Biosystems warrants at the time of release, this product conformed information contained in this certificate of analysis. The warranty provided herein is valid only when used by properly trained individuals. Unless otherwise stated in the Documentation, this warranty is limited to one year from date of shipment when the product is subjected to normal, proper and intended usage. The warranty extends only to the buyer of the product. Product is intended for research only and is not to be used for any other purpose, including unauthorized commercial uses, in vitro diagnostic uses, ex vivo or in vivo therapeutic uses, or any type of consumption by or application to humans or animals.