

CERTIFICATE OF ANALYSIS

Product: S-Adenosylhomocysteine (SAH) ELISA Kit Plasma

Catalog Number: IK00301

Lot Number:

SAH Assay Plate Lot#: 451027

HRP-anti-SAH antibody: Lot# 450204 & Lot#422024


Quality Release Date:

HRP-antibody Diluent	Tested earlier Lot # 422204
Sample Diluent	Tested earlier Lot # 422204
TMB Substrate	Tested earlier Lot # 422204
Stop Solution	Tested earlier Lot # 422204
SAH Standard	Tested earlier Lot # 451018
Wash Solution (20x)	Tested earlier Lot # 450407

HRP-anti-SAH antibody: Lot# 450204 1:750 & Lot#422024 1:1000

SAH Plasma Standard(nM)	Lot# 450204 1:750	Lot# 422024 1:1000
0	0.92725	1.14765
31.25	0.815	1.0445
62.5	0.74795	0.9419
125	0.64545	0.85015
250	0.541	0.64805
500	0.40585	0.48335
1000	0.29535	0.33465
Blank	0.0483	0.0472

Products are warranted to operate or perform substantially in conformance with published product data sheet in effect at the time of sale, as set forth in the product documentation, specifications and/or accompanying package inserts ("Documentation"). Arthus Biosystems warrants at the time of release, this product conformed information contained in this certificate of analysis. The warranty provided herein is valid only when used by properly trained individuals. Unless otherwise stated in the Documentation, this warranty is limited to one year from date of shipment when the product is subjected to normal, proper and intended usage. The warranty extends only to the buyer of the product. Product is intended for research only and is not to be used for any other purpose, including unauthorized commercial uses, in vitro diagnostic uses, ex vivo or in vivo therapeutic uses, or any type of consumption by or application to humans or animals.

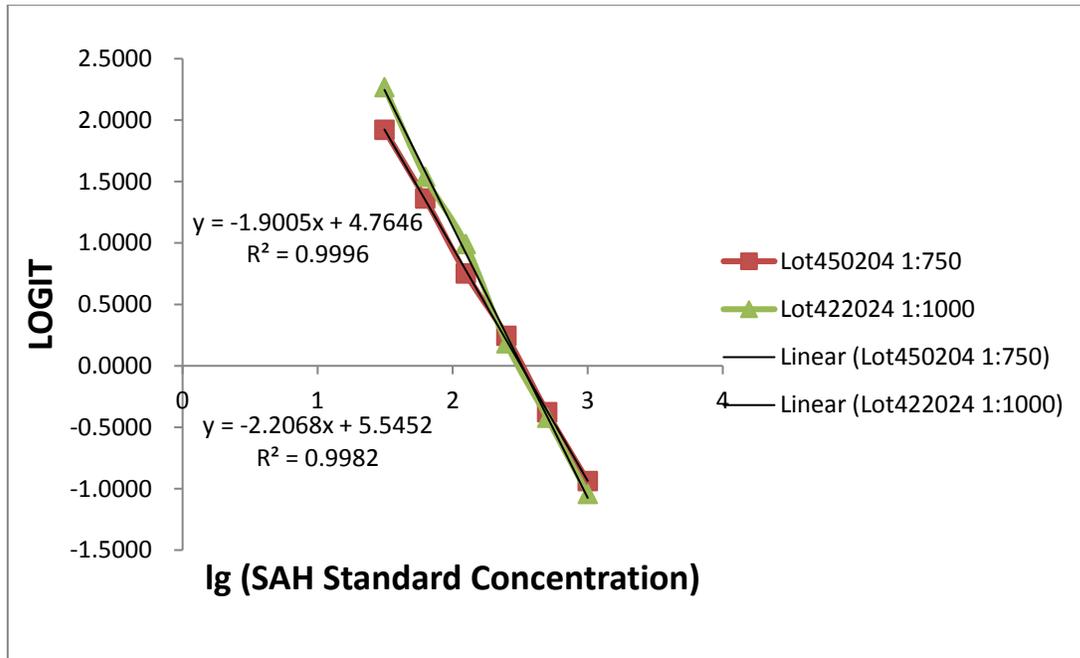

Jimmy Li
Quality Control Team

Products are warranted to operate or perform substantially in conformance with published product data sheet in effect at the time of sale, as set forth in the product documentation, specifications and/or accompanying package inserts ("Documentation"). Arthus Biosystems warrants at the time of release, this product conformed information contained in this certificate of analysis. The warranty provided herein is valid only when used by properly trained individuals. Unless otherwise stated in the Documentation, this warranty is limited to one year from date of shipment when the product is subjected to normal, proper and intended usage. The warranty extends only to the buyer of the product. Product is intended for research only and is not to be used for any other purpose, including unauthorized commercial uses, in vitro diagnostic uses, ex vivo or in vivo therapeutic uses, or any type of consumption by or application to humans or animals.